

Patient Name Date


Patient ID

Hospital Name Doctor Name

Comments




Gastroesophageal Junction Distensibility¹

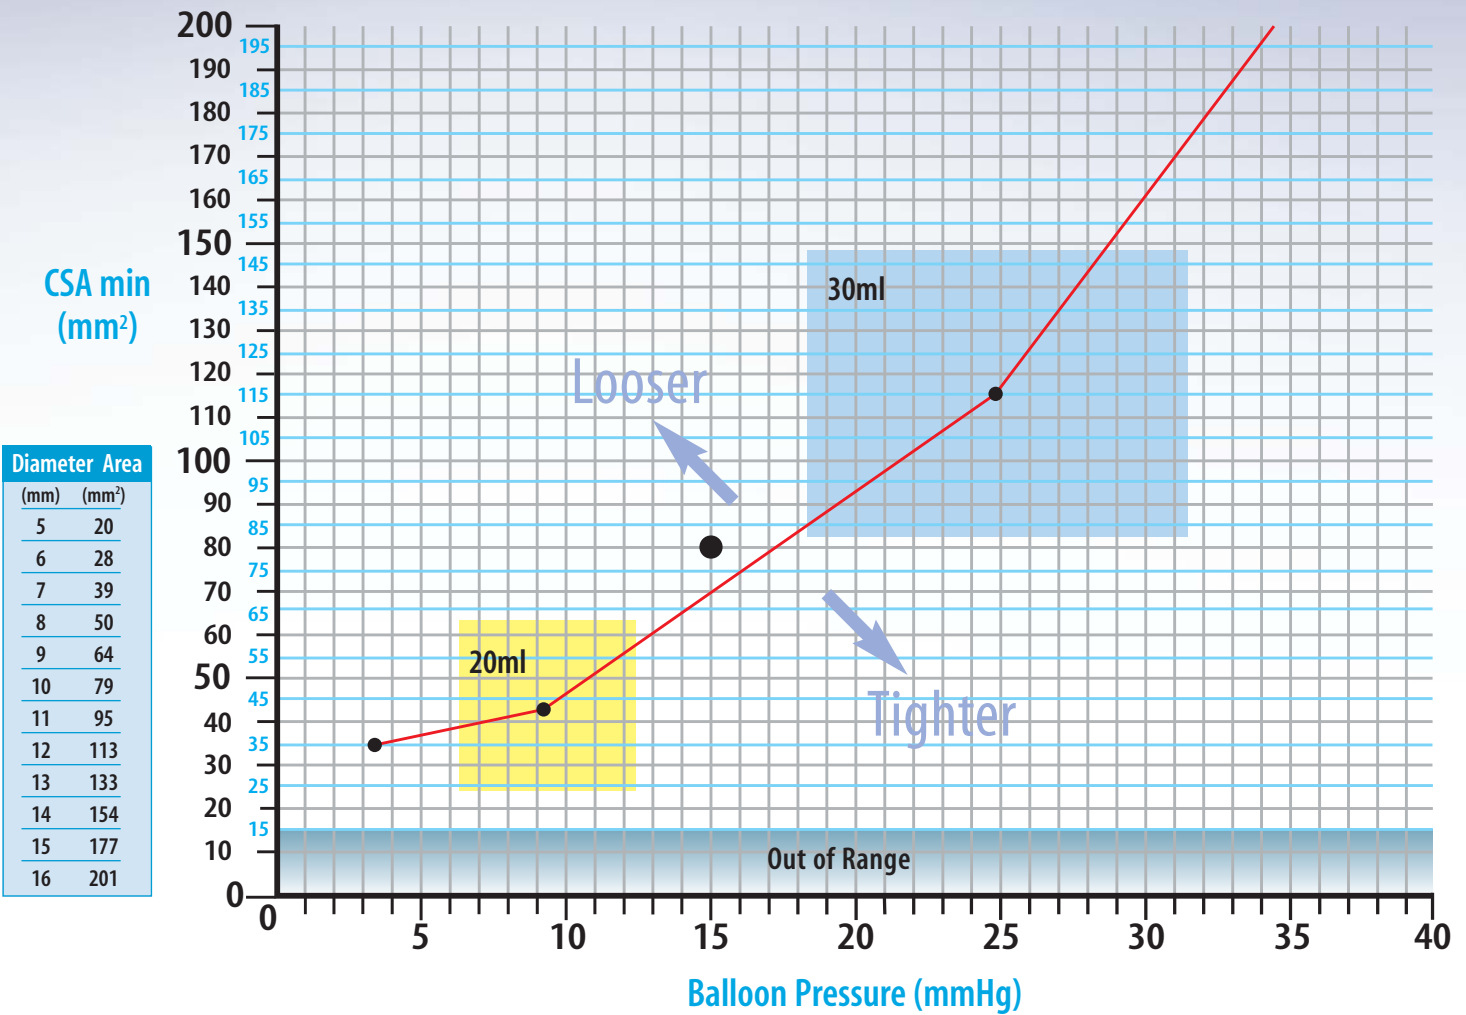

EndoFLIP Instructions

- Step ① Just prior to inserting the catheter in the patient, place the balloon on a flat surface, and zero the pressure sensor with approx. 2-3mL in the balloon.
- Step ② Introduce the catheter to the **centre** of the GEJ.
- Step ③ Inflate the balloon to 30mL, and ensure an hourglass figure is obtained with the minimum diameter being to the middle part of the balloon. Note the balloon pressure (P) and minimum cross-sectional area (CSA min). Plot **CSA Min** versus **Pressure** on the graph above.
- Step ④ Repeat Step 3 for 20mL balloon volume.

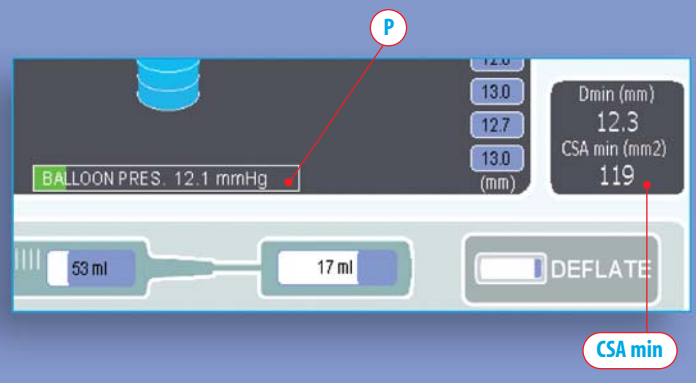

¹Increased Esophagogastric Junction Distensibility in GERD Patients Assessed with the Endoscopically Placed Functional Luminal Imaging Probe (Endoflip[®])
Monika A. Kwiatek, Ikuo Hirano, Peter J. Kahrlas, Barry P. McMahon, John E. Pandolfino Gastroenterology May 2009 (Vol. 136, Issue 5, Page A-16)

Patient Name Date


Patient ID

Hospital Name Doctor Name

Comments




Gastroesophageal Junction Distensibility¹

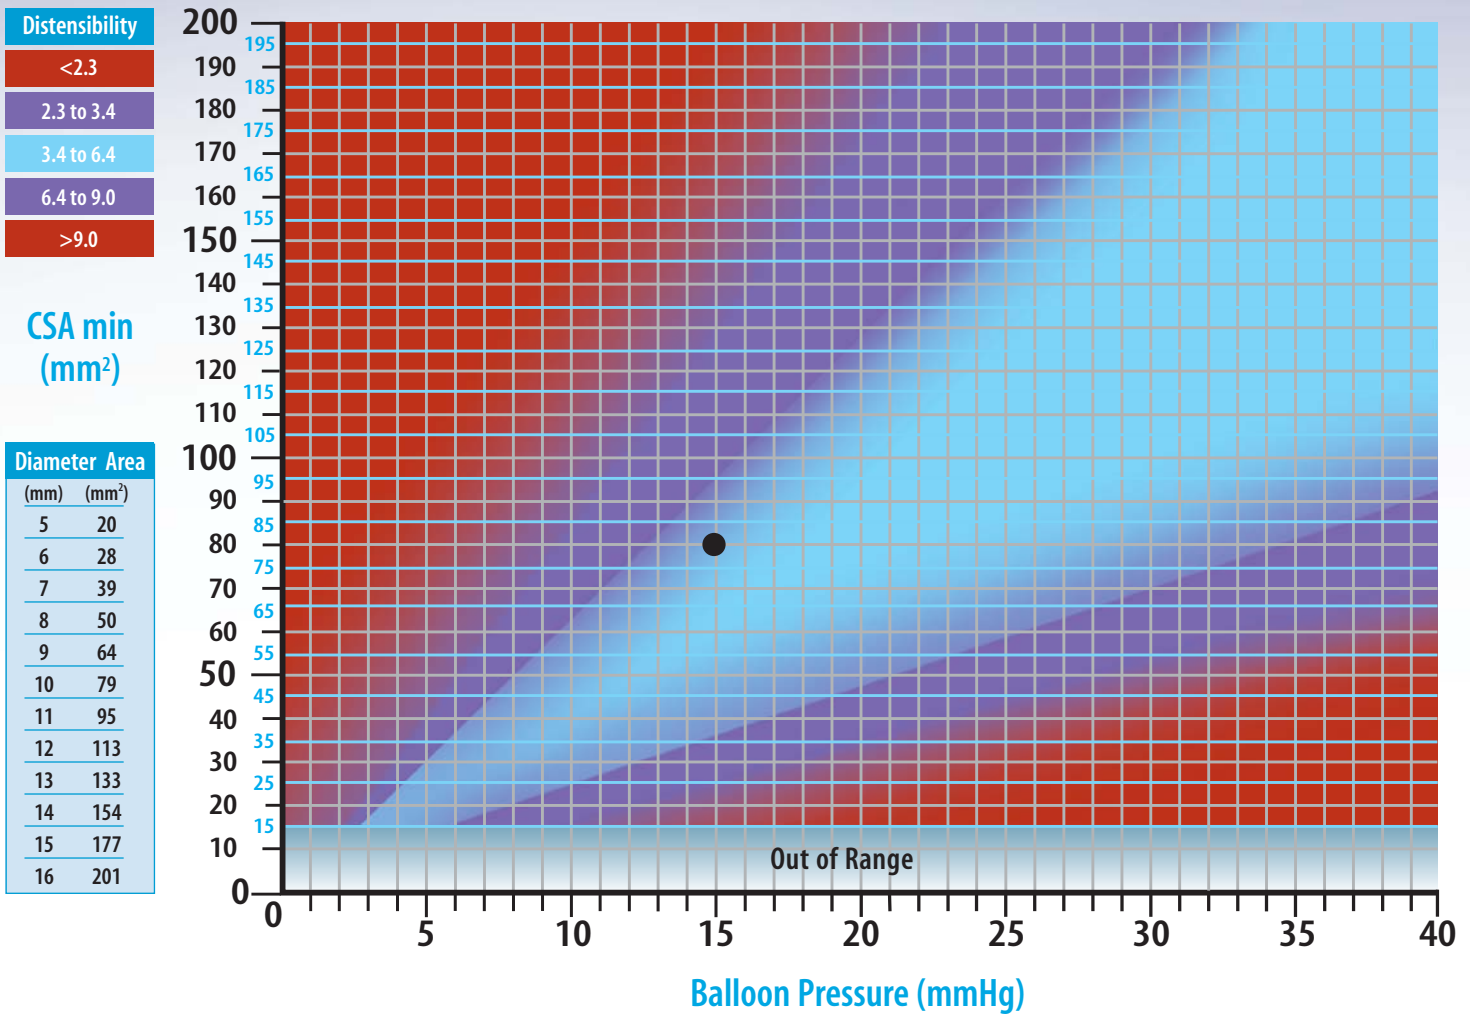

EndoFLIP Instructions

- Step ① Just prior to inserting the catheter in the patient, place the balloon on a flat surface, and zero the pressure sensor with approx. 2-3mL in the balloon.
- Step ② Introduce the catheter to the **centre** of the GEJ.
- Step ③ Inflate the balloon to 30mL, and ensure an hourglass figure is obtained with the minimum diameter being to the middle part of the balloon. Note the balloon pressure (P) and minimum cross-sectional area (CSA min). Plot **CSA Min** versus **Pressure** on the graph above.
- Step ④ Repeat Step 3 for 20mL balloon volume.

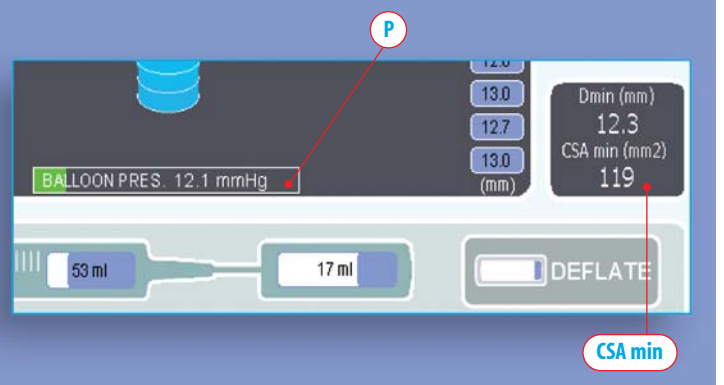

¹Increased Esophagogastric Junction Distensibility in GERD Patients Assessed with the Endoscopically Placed Functional Luminal Imaging Probe (Endoflip®)
Monika A. Kwiatek, Ikuo Hirano, Peter J. Kahrlas, Barry P. McMahon, John E. Pandolfino Gastroenterology May 2009 (Vol. 136, Issue 5, Page A-16)